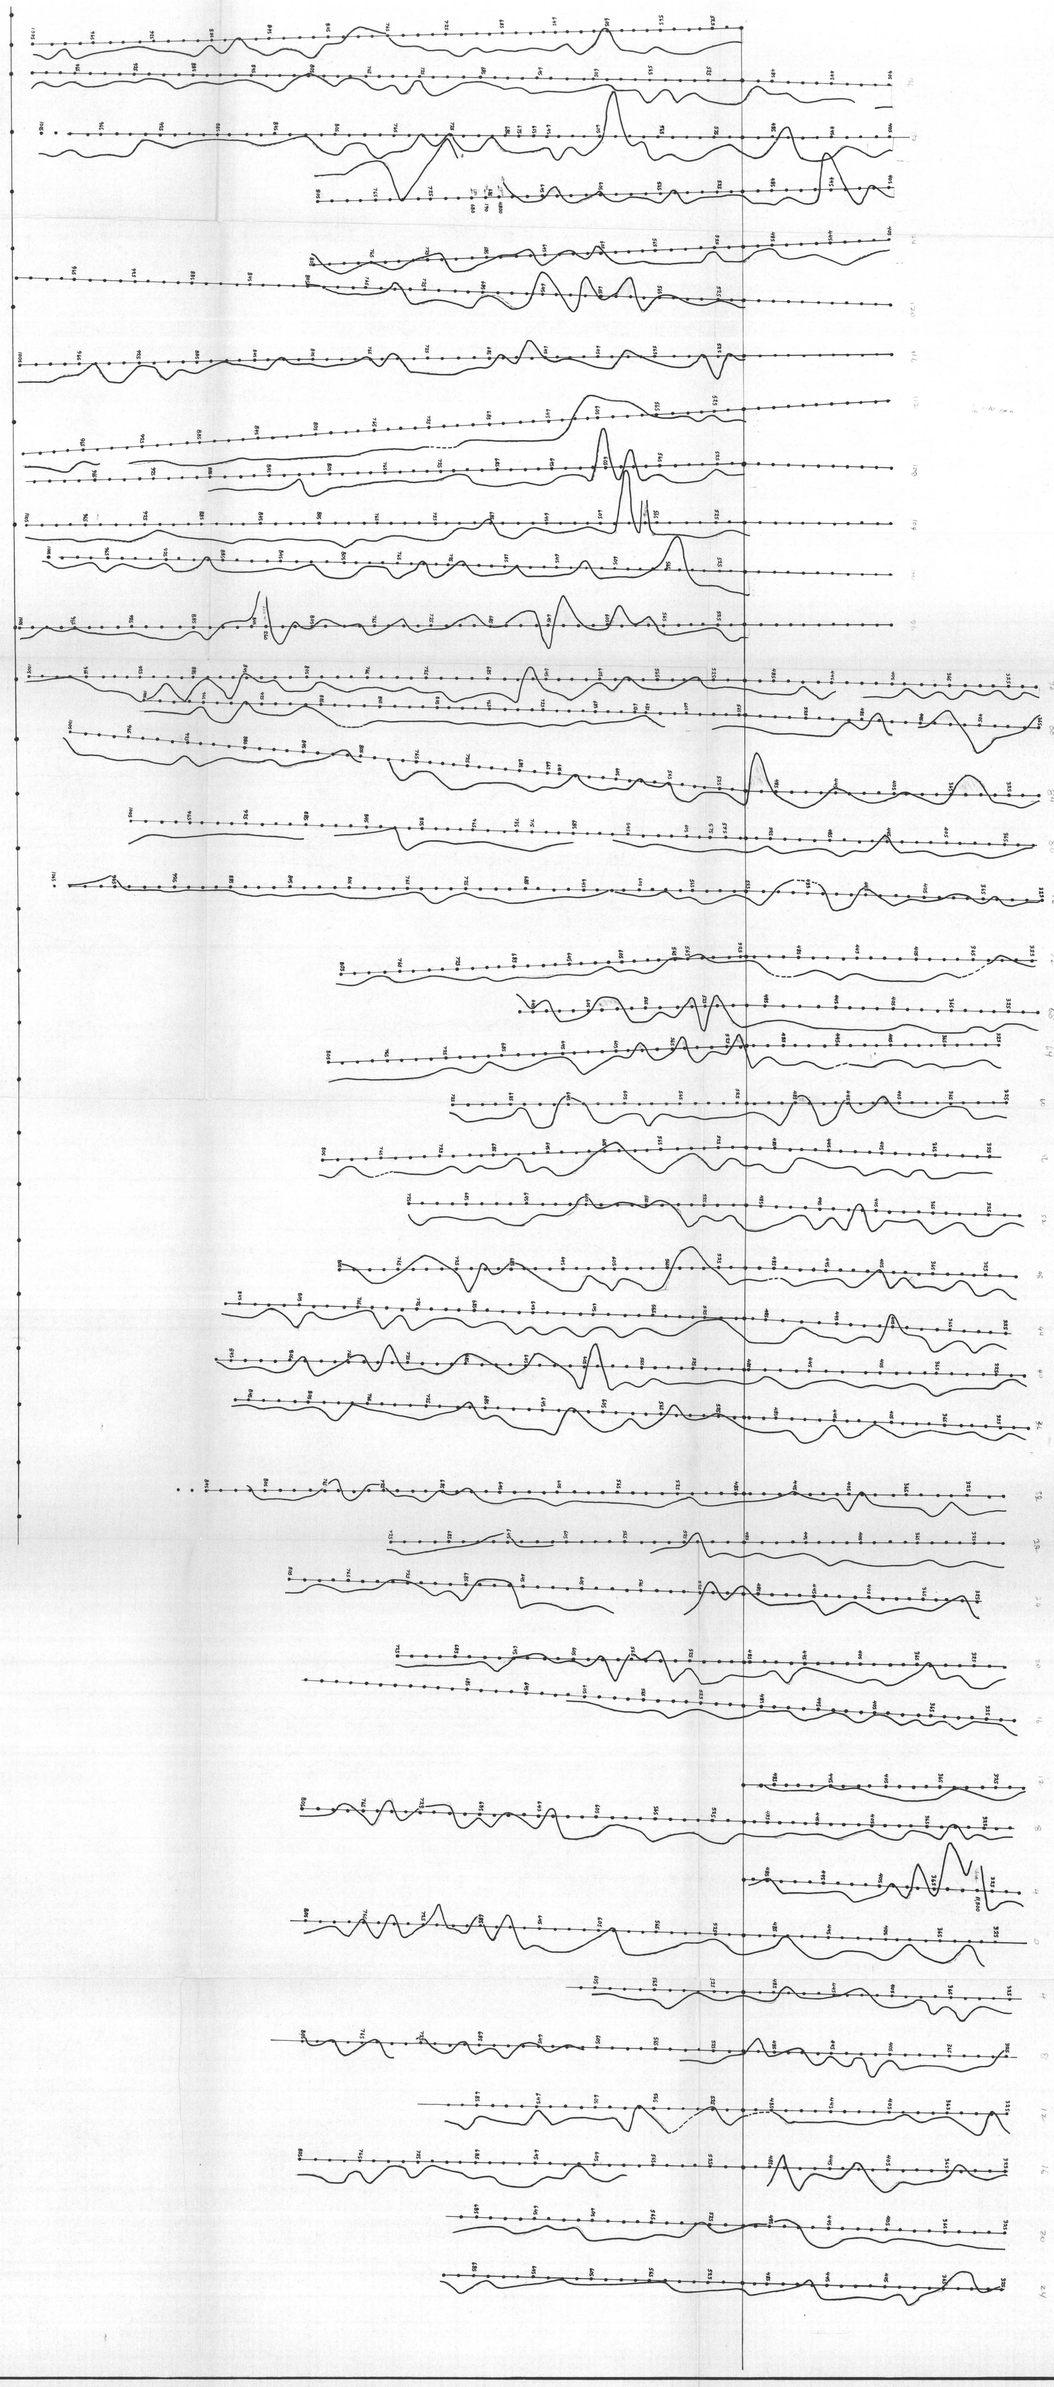

Geophysical Service Inc.
Texas Instruments
Dallas, Texas
Seismograph Record
Shot Point 1
Shot Date 1-2-58
Shot Time 1:00 AM
Shot Depth 50 Feet
Shot Charge 50 Lbs.
Gain 60 DB
Filter 30-60 CPS
Time
0
1
2
3
4
5

014177